

CareStart COVID-19 Antigen Test Competency Quiz





Return this form to MDHHS Bureau of Laboratories at anglewiczc@michigan.gov or fax 517-335-9631

Trainee Name (Please Print) _____

Facility Name (Please Print) _____ Date _____

Trainees must achieve at least 80% (4/5 correct answers) to successfully complete this training. MDHHS Bureau of Laboratories will contact those who need additional assistance.

1. What is the time range that the CareStart Antigen test can be interpreted after beginning the test?
 - a. 5-10 minutes
 - b. 10-15 minutes
 - c. 10-20 minutes
 - d. 15-30 minutes
2. Interpret the results of the tests below by circling the correct answer:

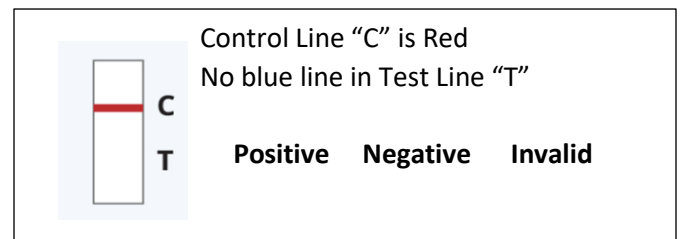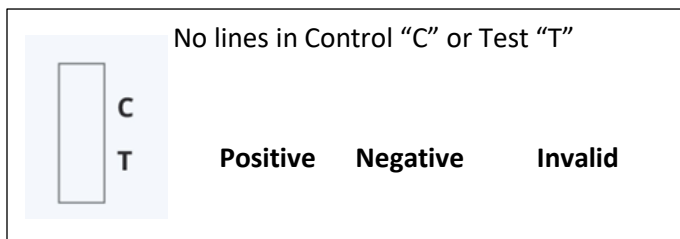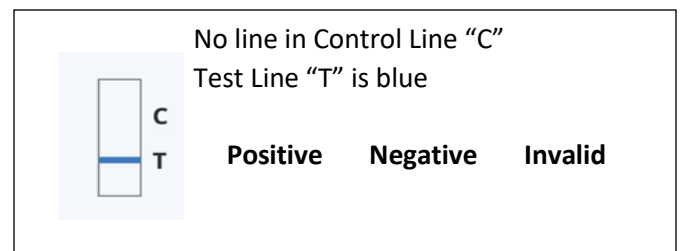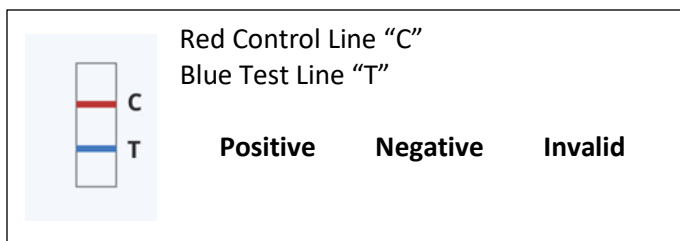

3. **True** or **False** (Circle correct answer) A faint blue "T" test line is considered a positive result (the control line present)
4. **True** or **False** (Circle correct answer) A nasopharyngeal swab must be collected by trained personnel
5. **True** or **False** (Circle correct answer) It is ok to discard contaminated gloves and other testing materials in regular waste instead of a biohazard waste container.